




Config1. (should arrive to last diff. S2D2 with UHV chamber) M1=M2=2.13 mrad, Mono1=20 mm offset, Mono2=15 mm offset  
 Config2. (should arrive to last diff. S2D2 with UHV chamber) M1=M2=2.13 mrad, Mono1=20 mm offset, No mono2  
 Config3. (should arrive to SiXC diff, i.e., first diff in EH2) M1=2.13, M2=2.72 mrad, Mono1=20 mm offset, No Mono2  
 Config4. (should arrive to diff in EH1. No matter if the beam does not enter in EH2) M1=2.13, M2=3.89 mrad, Mono1=20 mm offset, No Mono2  
 Config5. (should arrive to SiXC diff, i.e., first diff in EH2) M1=2.72, M2=2.72 mrad, Mono1=20 mm offset, No Mono2  
 Config6. (should arrive to diff in EH1. No matter if the beam does not enter in EH2) M1=3.89, M2=3.89 mrad, Mono1=20 mm offset, No Mono2  
 Config7. (should arrive everywhere). M1=0, M2=0 mrad, Mono1=20 mm offset, No Mono2  
 Config8. (should arrive everywhere). M1=0, M2=0 mrad, Mono1=20 mm offset, Mono2=15 mm offset

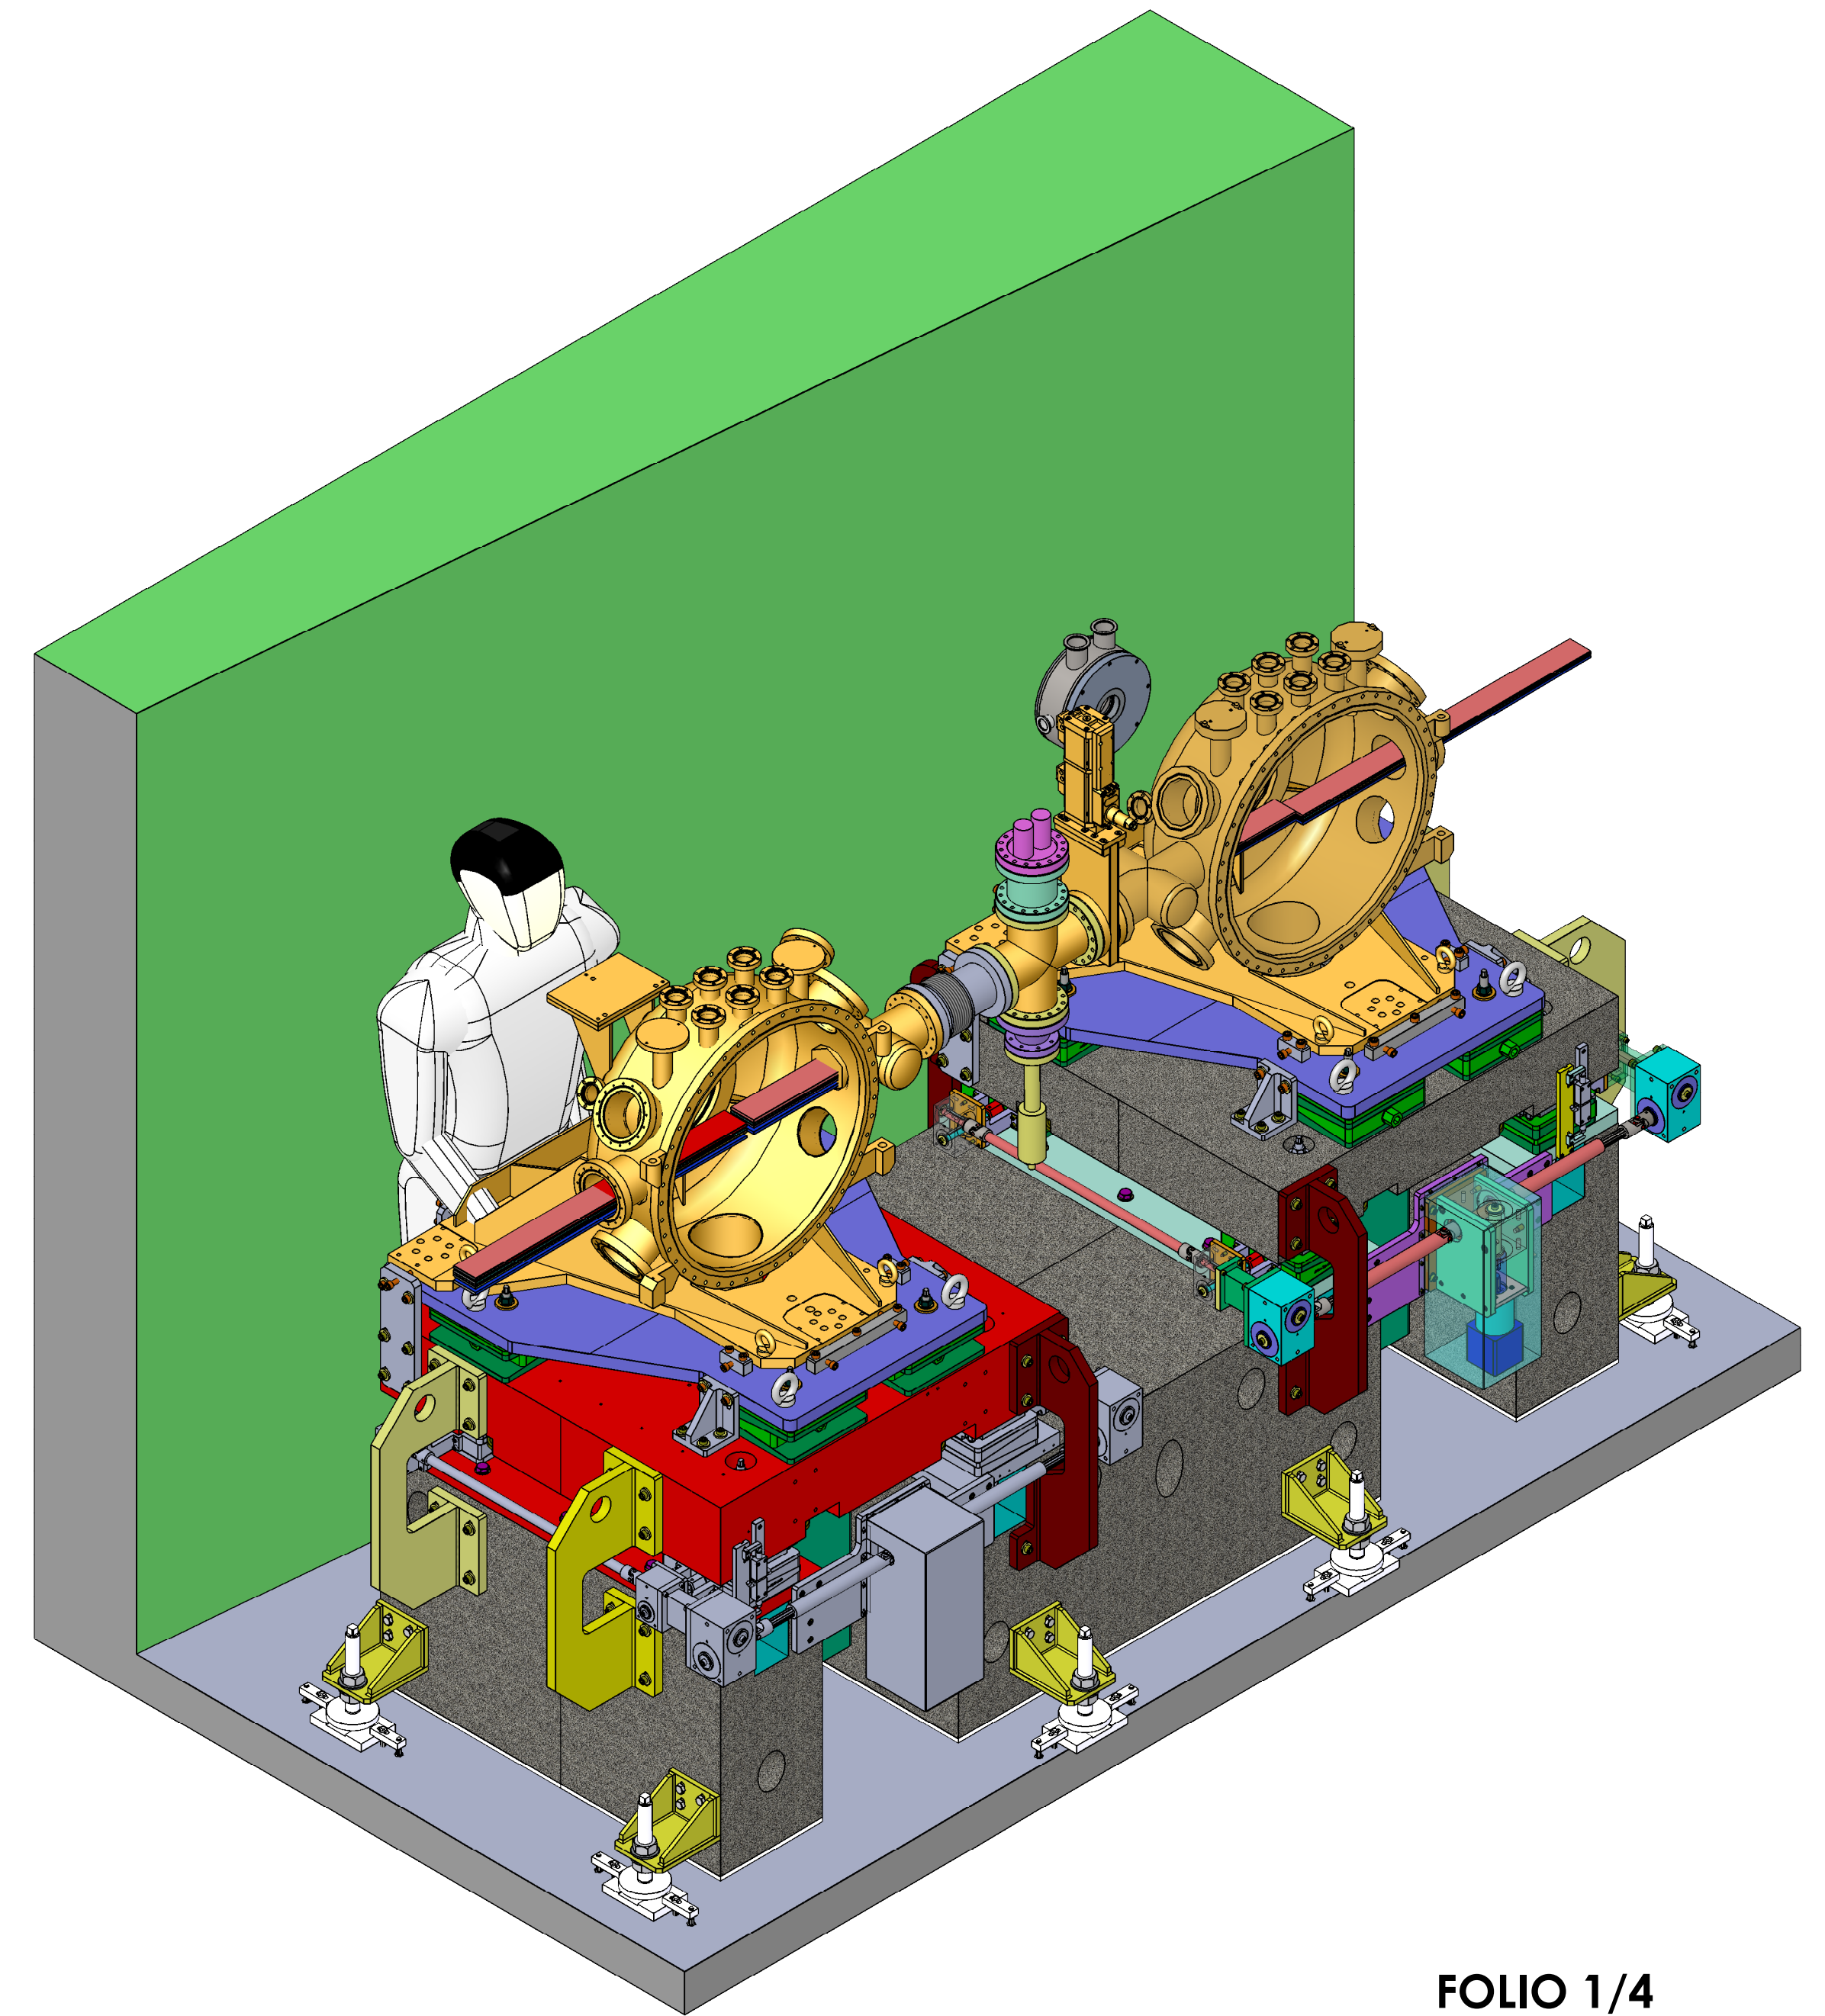

**FOLIO 1/4**

Position montage  
Hauteur mediane des airloc  
Pièces grises: Existantes  
Pièces rouge: Modifiées, ajout trous  
Autres couleurs: Nouvelles pièces

ITEM	DRAWING N.	QTY	DESCRIPTION /	REMARKS	MATERIAL	W./Kg
0mm	SCALE:		100	DRN. CKD. APPD.	NAME	DATE
				ISO STANDARD		
				GEN. SURFACE FINISH :		
				GEN. LINEAR TOL. :		
				GEN. ANGULAR TOL. :		
				ASSY.		
<div>   <div> <b>Spanish CRG Beamline</b>            AT EUROPEAN SYNCHROTRON            BP 220 38043 GRENOBLE CEDEX-FRANCE            Comisión Interministerial de Ciencia y Tecnología CICYT            C/ Rosario Pino 14-16 28020 MADRID - ESPAÑA         </div> </div>						
A1			10	11	12	SolidWorks